

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606




Date: 09/13/2023

LEB

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:23
INTERNAL STANDARD	VERIFIED	23:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:23
BLANK TEST	0.00	23:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:25
BLANK TEST	0.00	23:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:26
BLANK TEST	0.00	23:27

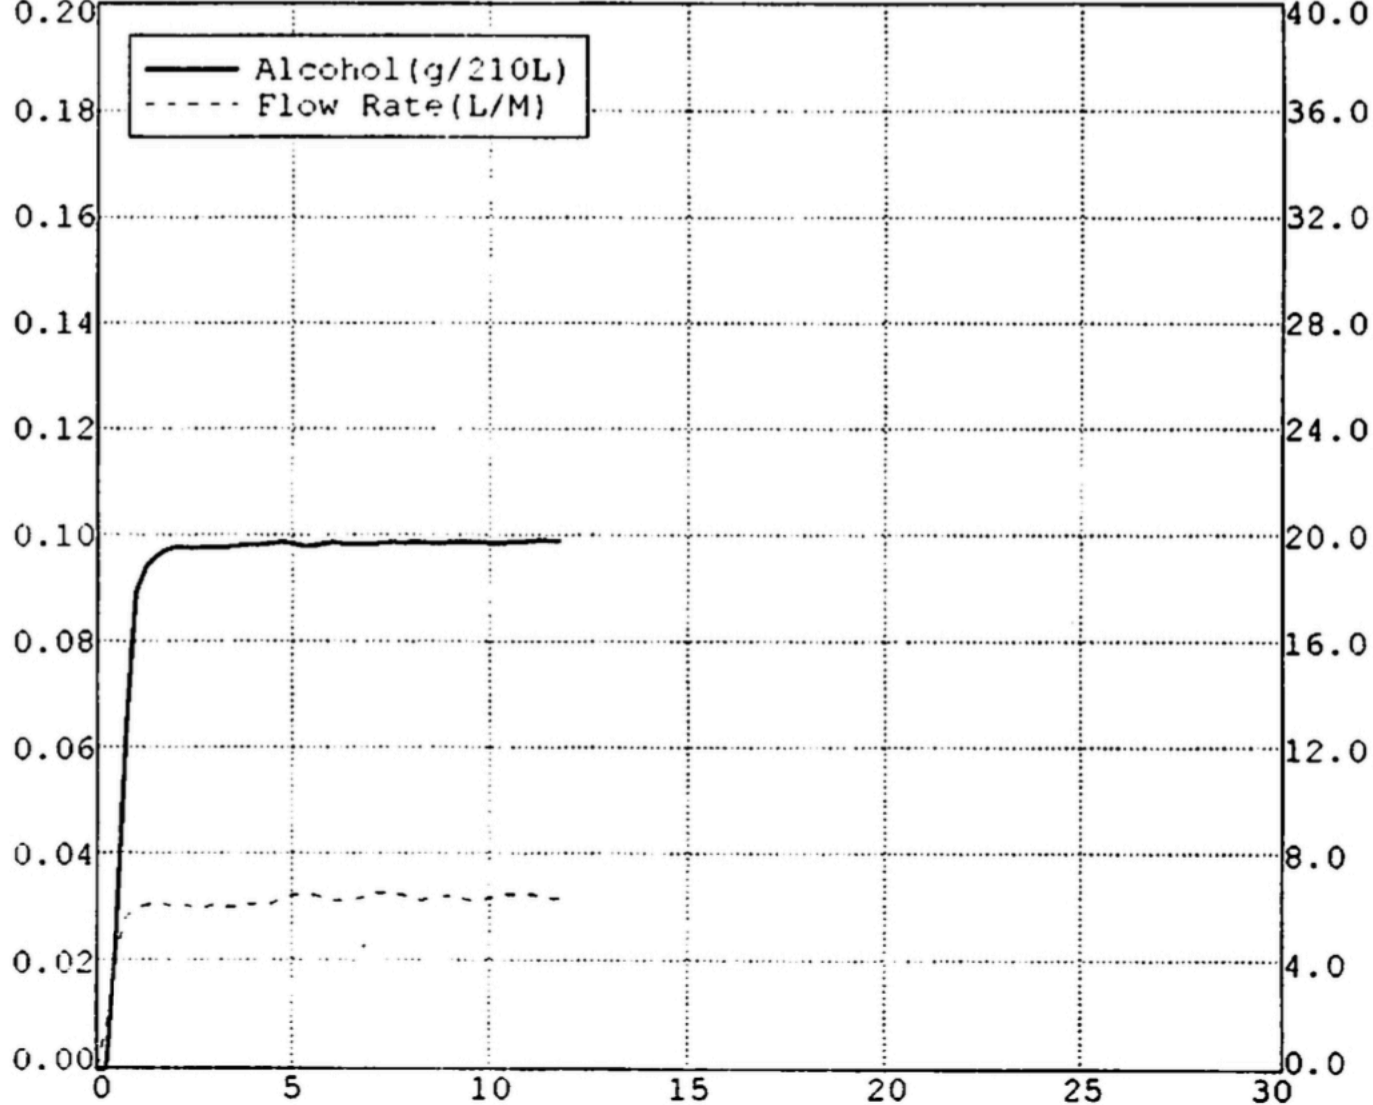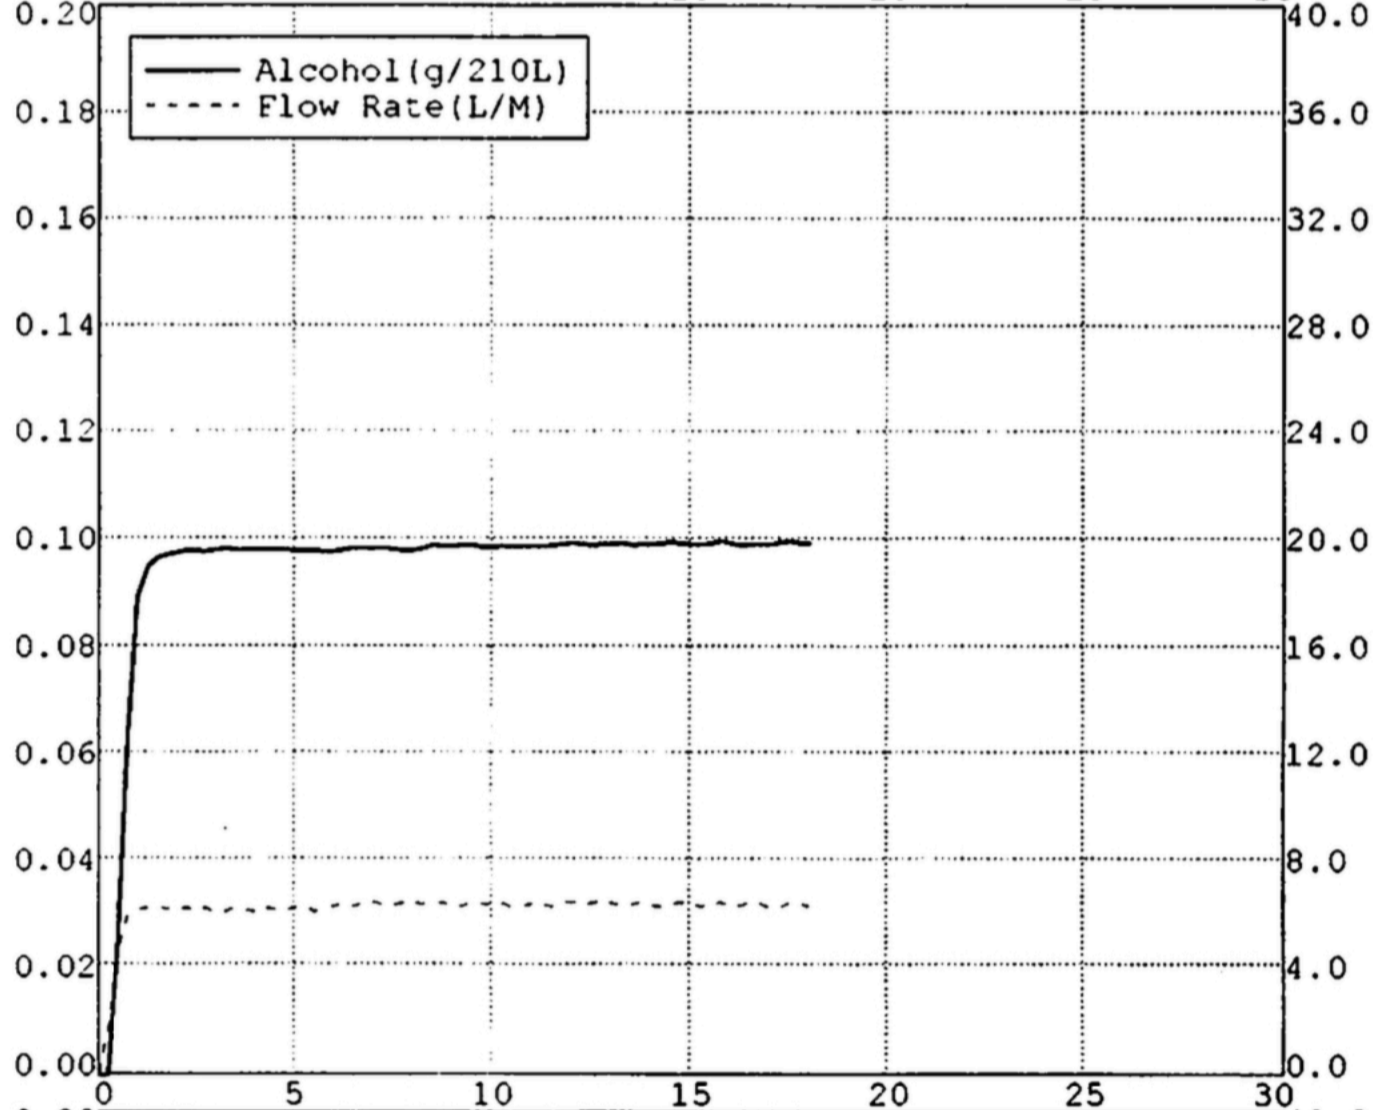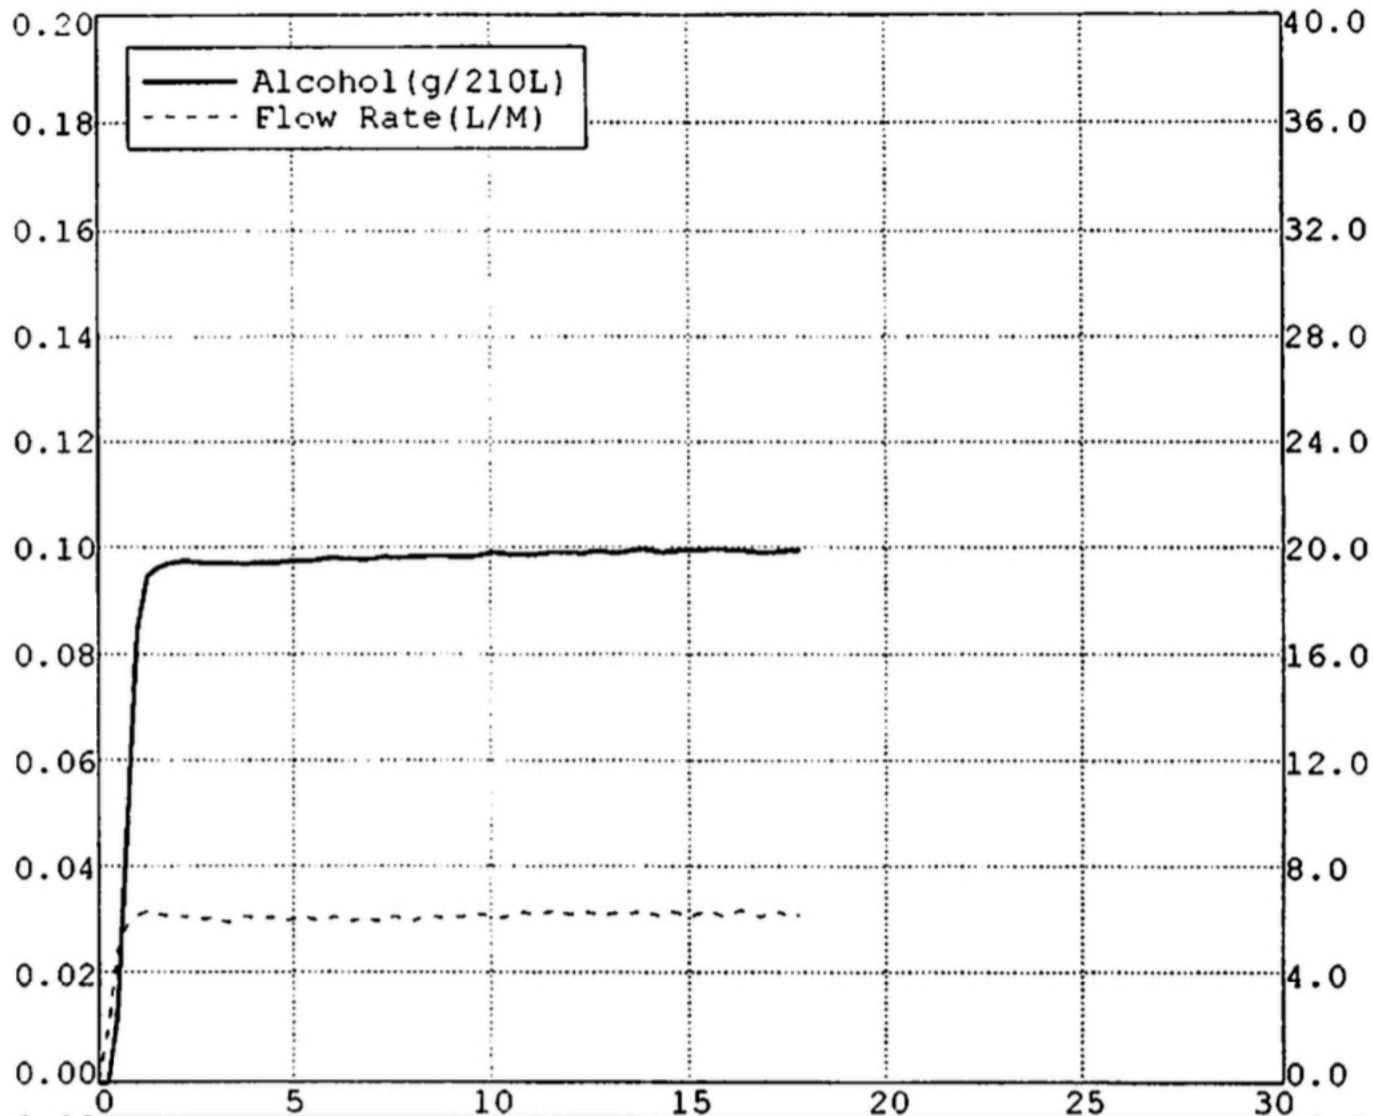

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

LEB

Date: 09/13/2023

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 23190

Nominal = 0.10 g/210L

RFI Detected