

SUPERVISOR TEST




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 07/19/2023

OPERATOR NAME:
BAILEY J DIXON
Permit #: 50814
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:09
INTERNAL STANDARD	VERIFIED	01:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:10
BLANK TEST	0.00	01:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:11
BLANK TEST	0.00	01:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:12
BLANK TEST	0.00	01:13

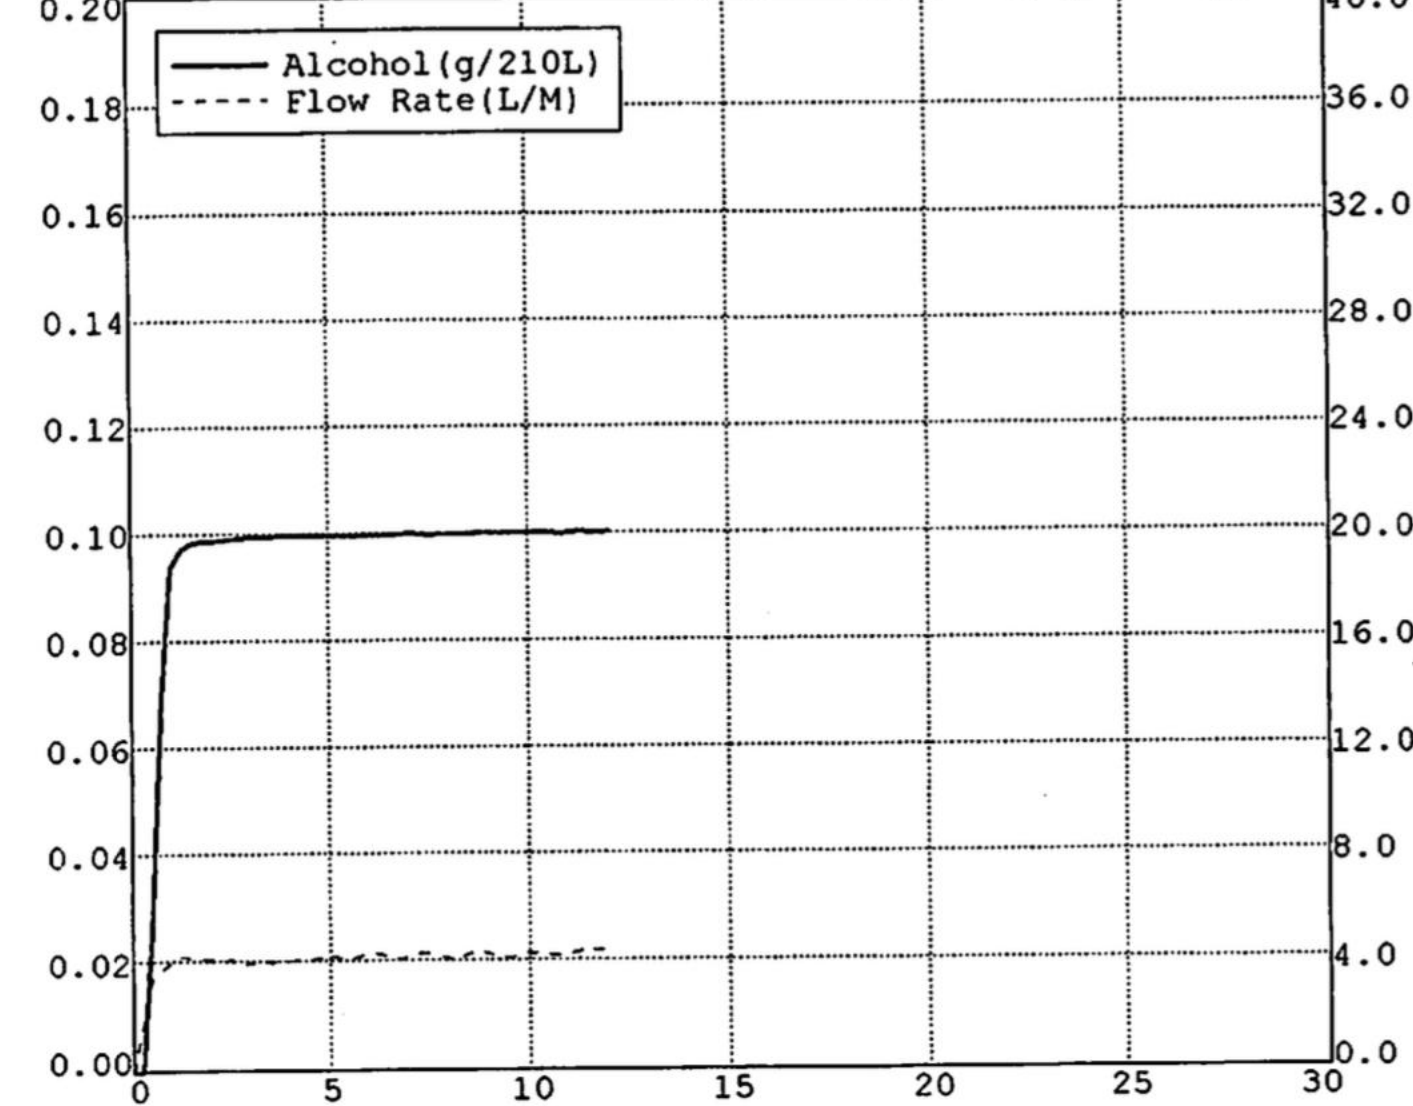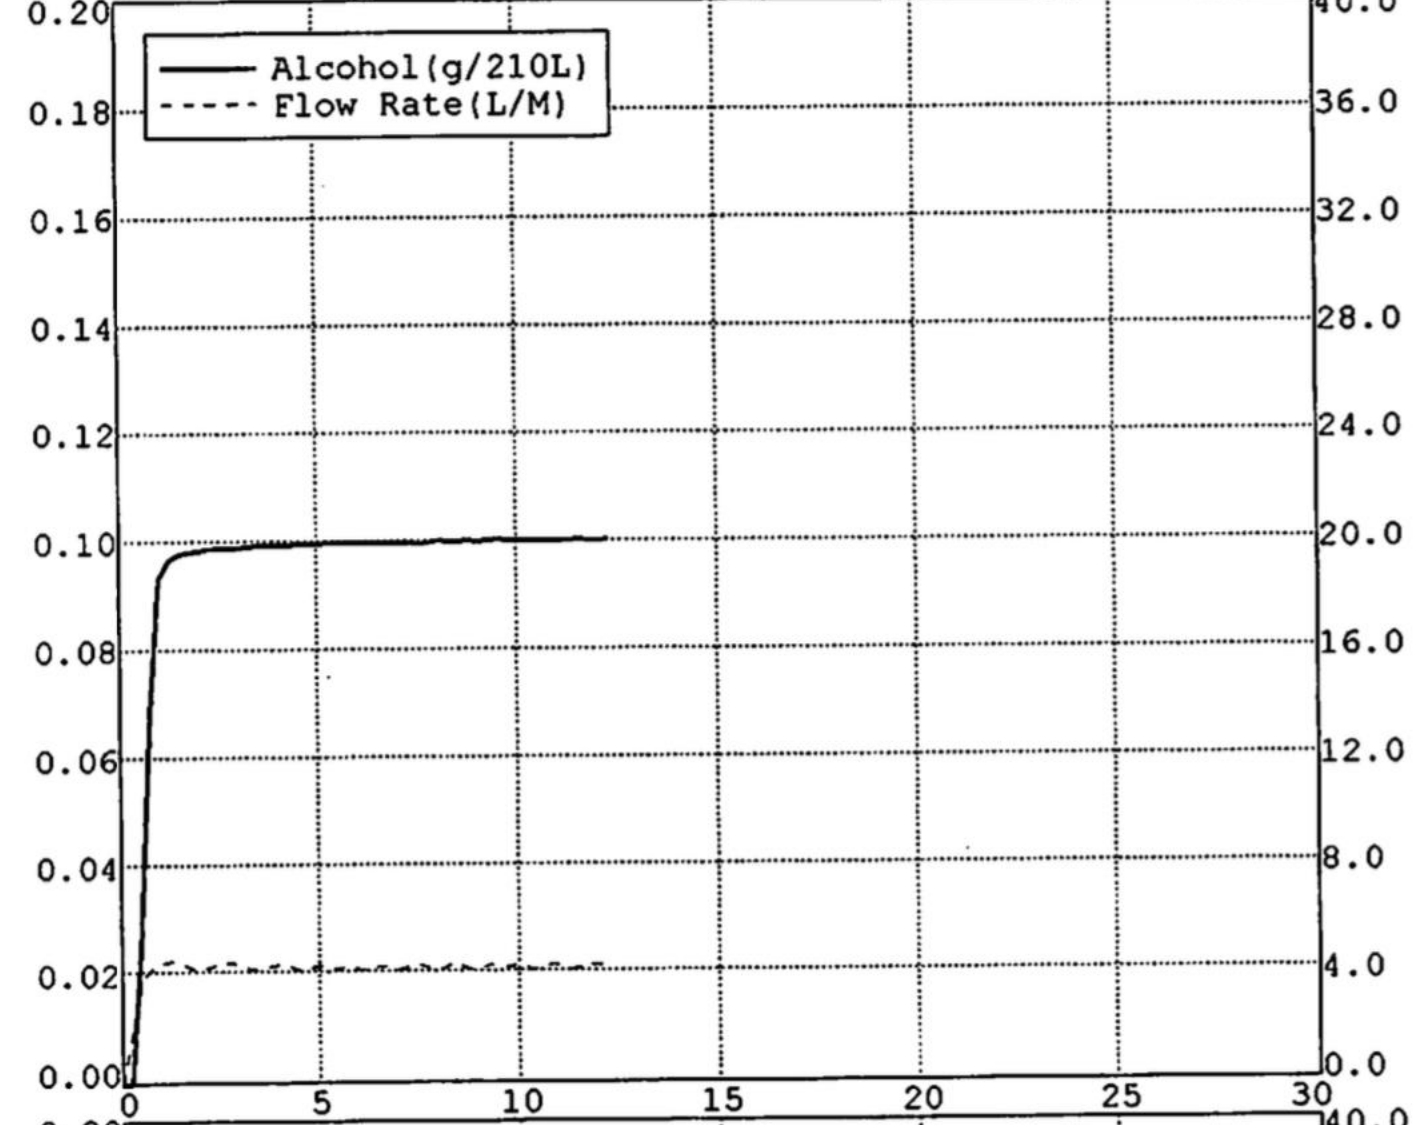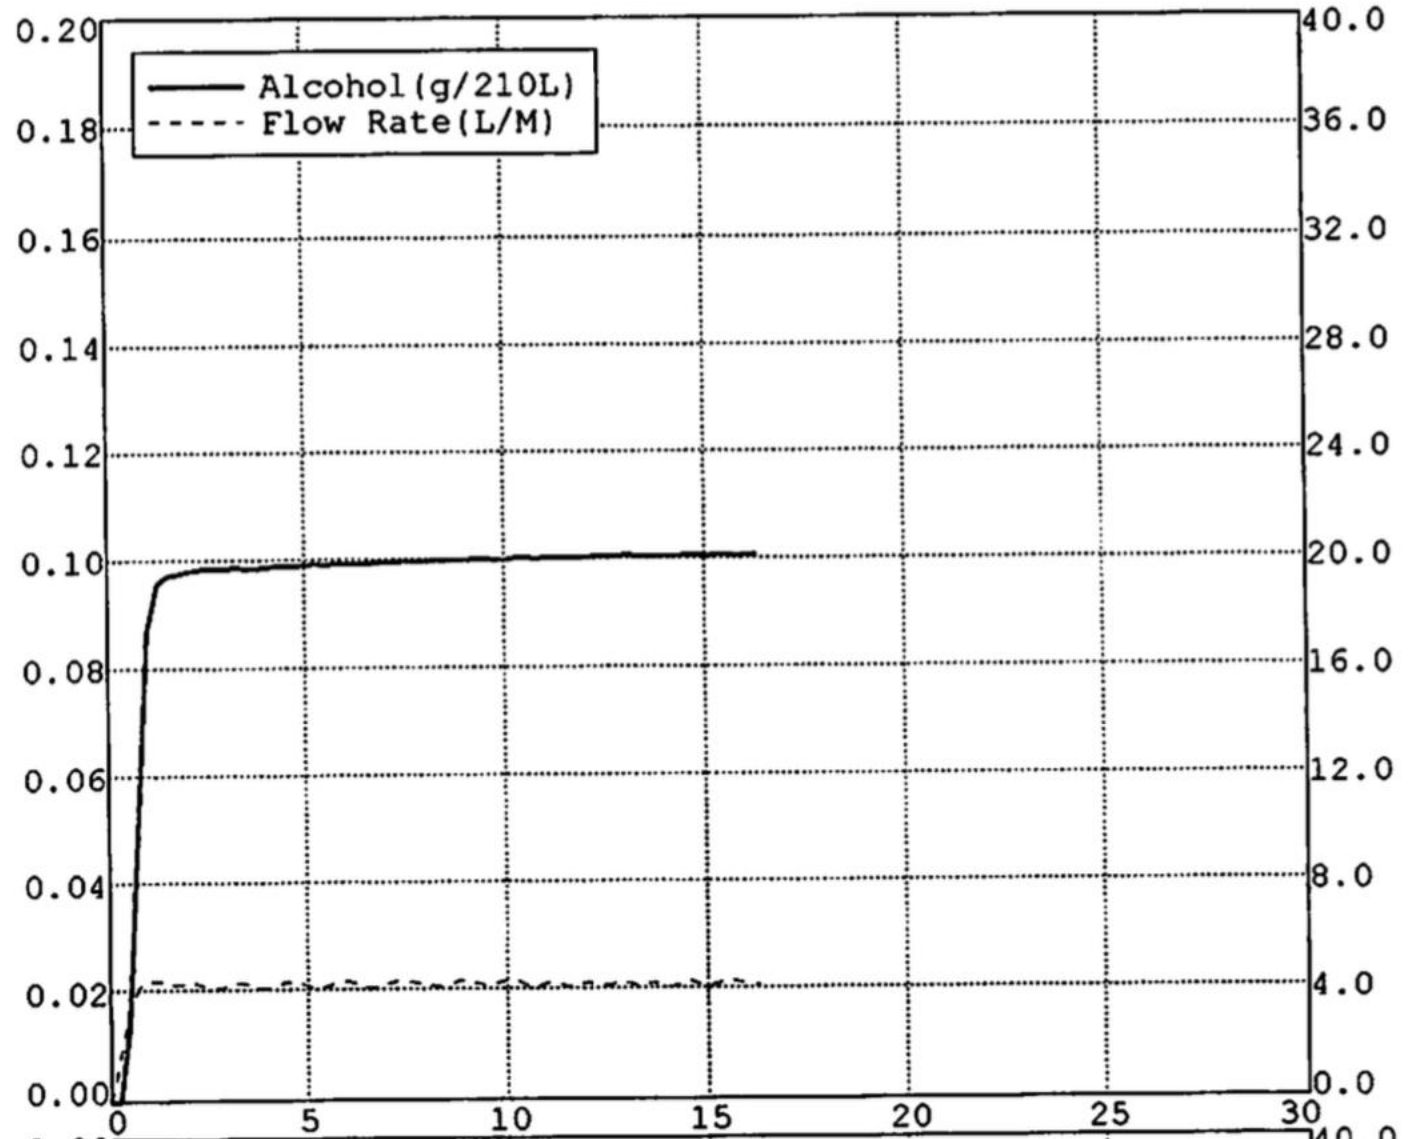

SUPERVISOR TEST

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 07/19/2023

OPERATOR NAME:
BAILEY J DIXON
Permit #: 50814
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:09
INTERNAL STANDARD	VERIFIED	01:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:10
BLANK TEST	0.00	01:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:11
BLANK TEST	0.00	01:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:12
BLANK TEST	0.00	01:13

