

SUPERVISOR TEST

650




ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

Date: 01/03/2024

OPERATOR NAME:  
JASON L OSIKA  
Permit #: 35567  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 23350

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 01:20 |
| INTERNAL STANDARD       | VERIFIED | 01:20 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 01:21 |
| BLANK TEST              | 0.00     | 01:22 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 01:22 |
| BLANK TEST              | 0.00     | 01:23 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 01:23 |
| BLANK TEST              | 0.00     | 01:24 |

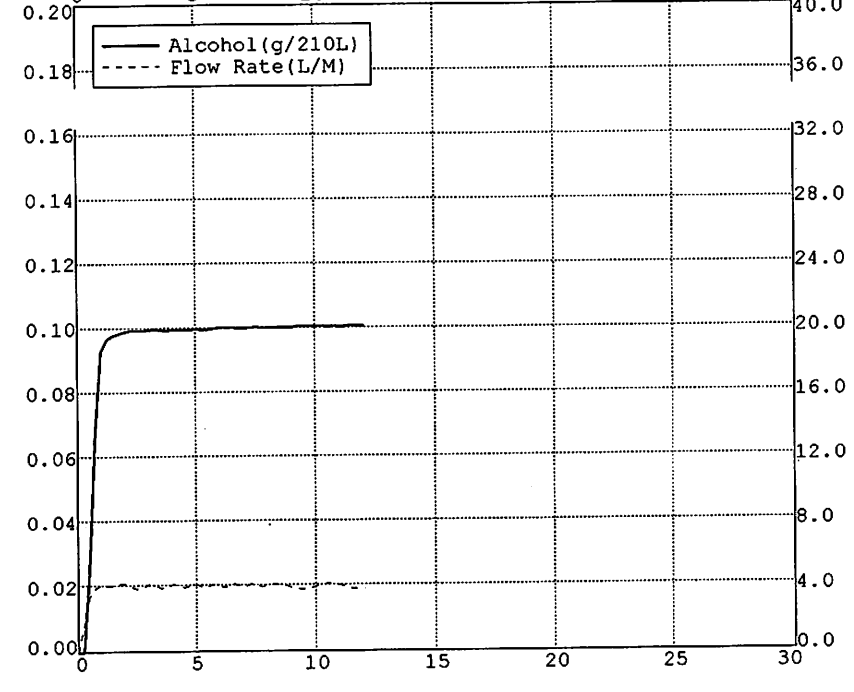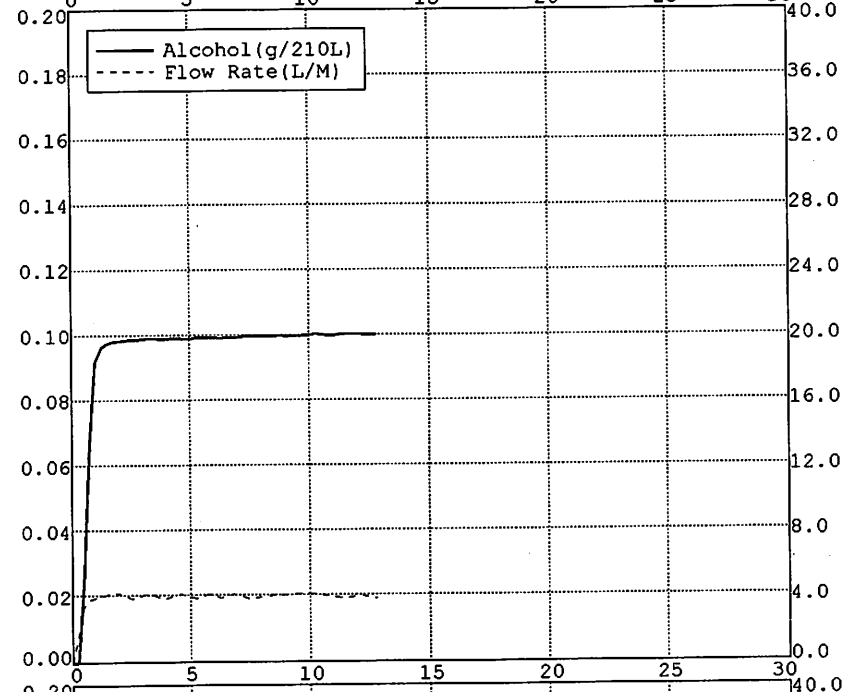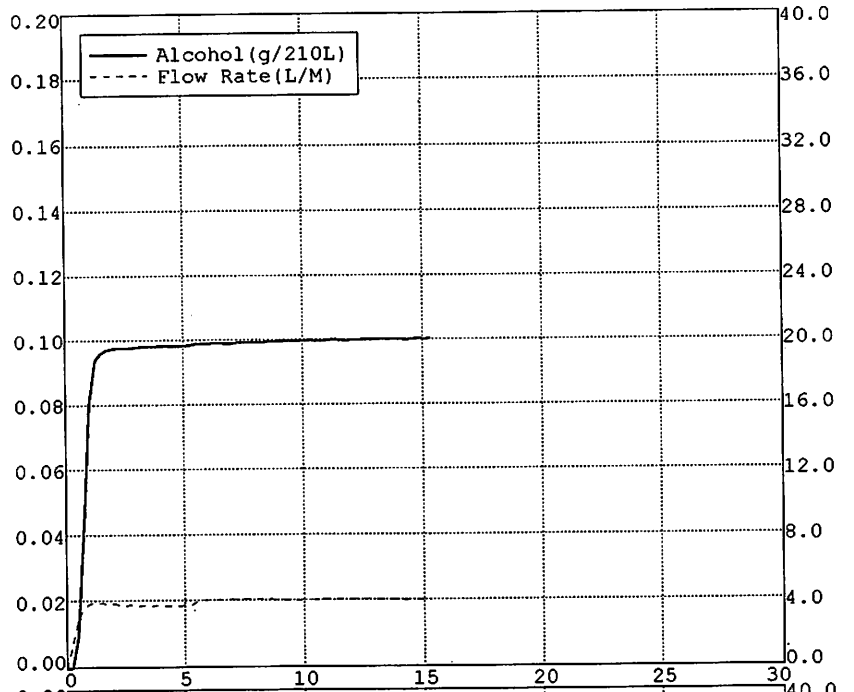

U ↓ - ↓ -